

INSTALLATION INSTRUCTION



CONCEALED SHOWER

| IAPMO RESEARCH AND TESTING, INC. | |
|--|----------------------------|
| CERTIFICATE OF LISTING | |
| Issued To: QIANG YING HOSE FACTORY | Effective Date: April 2021 |
| File Number: N-12908 | |
| NSF/ANSI/CAN 61 | |
| Product: Drinking Water System Components - Health Effects | Valid After: April 2026 |
| This certificate is not evidence of current listing. To verify listing status, visit the IAPMO R&T Product Listing Directory at pds.iapmo.org | |
| Identification: Each product shall be permanently and legibly marked with the manufacturer's name or trademark. The product may also be marked with the standard designation "NSF/ANSI/CAN 61". | |
| Characteristics: Materials or products that come into contact with drinking water and/or drinking water treatment chemicals. Products and materials may include process metals, protective linings, joining and joining materials, pipes and related products, mechanical devices used with treatment/transmission/distribution systems, and mechanical plumbing devices. To be installed in accordance with the manufacturer's instruction. Lead free requirements are addressed under a separate certificate of listing. | |
| Products listed on this certificate have been tested by an IAPMO R&T recognized laboratory. This recognition has been granted based upon the laboratory's compliance to the applicable requirements of ISO/IEC 17025. | |

Page 2 of 4

IAPMO R&E WORKING GROUP

IAPMO RESEARCH AND TESTING, INC.

5001 E. Philadelphia Street, Ontario, CA 91761-2916 • Fax (909) 472-4200 • Fax (909) 472-4244 • www.iapmrt.org





IAPMO R&T Product Listing

This IAPMO R&T listing is current as of 8/22/2020



C

Product

Manufacturer

Model Number

Material

Finish

Color

Notes

Dimensions

Weight

Volume

Flow Rate

Pressure Drop

Installation

Maintenance

Warranty

Other Information

Flushing Fixture Fittings

WEISSER, INC.

11 HERRINGTON HEIGHTS

WATSONVILLE, CA 95070

Identification:

The flushing component shall have permanent labeling markings to identify the manufacturer. This marking shall be the same size, typeface, or other mark known to identify the manufacturer. The product shall have all other markings required by the standards. The marking shall be placed where it can be readily seen after installation to complete the product or packaging shall also bear the UPDM certification mark.

Characteristics:

The flushing fixture fitting component to be installed in accordance with the Manufacturer's instructions and the requirements of the latest edition of the Uniform Plumbing Code. Products listed on this certificate have been tested by an IAPMO R&T recognized laboratory. This recognition has been based solely upon the laboratory's compliance to the applicable requirements of ASSE 1001.

Products are in compliance with the following code(s):

- Uniform Plumbing Code (UPC)
- National Plumbing Code (NPC)
- International Plumbing Code (IPC)

Products are in compliance with the following standard(s):

ASSE A112.1-1-2016/CSA B12.1-14

NOTES:

Castell, Chromastep, Chromastep, HERRINGER, JOM, Kallisto, Spring Fish, Ten Thousand, Tivoli, Chromatic Supreme

Accessory Part Number: 30mm x 1/2in x 1/2in x 1/2in

(A) Assembly Type

- 1 Assembly
- 2 Plastic Brass Adapter
- 3 Check

(B) Product Type

- 1 Inlet
- 2 Inlet
- 3 Outlet
- 4 Valve
- 5 Drain
- 6 Spring Pin
- 7 Inlet
- 8 Inlet
- 9 Inlet
- 10 Inlet
- 11 Inlet
- 12 Inlet
- 13 Inlet
- 14 Inlet
- 15 Inlet
- 16 Inlet
- 17 Inlet
- 18 Inlet
- 19 Inlet
- 20 Inlet
- 21 Inlet
- 22 Inlet
- 23 Inlet
- 24 Inlet
- 25 Inlet
- 26 Inlet
- 27 Inlet
- 28 Inlet
- 29 Inlet
- 30 Inlet
- 31 Inlet
- 32 Inlet
- 33 Inlet
- 34 Inlet
- 35 Inlet
- 36 Inlet
- 37 Inlet
- 38 Inlet
- 39 Inlet
- 40 Inlet
- 41 Inlet
- 42 Inlet
- 43 Inlet
- 44 Inlet
- 45 Inlet
- 46 Inlet
- 47 Inlet
- 48 Inlet
- 49 Inlet
- 50 Inlet
- 51 Inlet
- 52 Inlet
- 53 Inlet
- 54 Inlet
- 55 Inlet
- 56 Inlet
- 57 Inlet
- 58 Inlet
- 59 Inlet
- 60 Inlet
- 61 Inlet
- 62 Inlet
- 63 Inlet
- 64 Inlet
- 65 Inlet
- 66 Inlet
- 67 Inlet
- 68 Inlet
- 69 Inlet
- 70 Inlet
- 71 Inlet
- 72 Inlet
- 73 Inlet
- 74 Inlet
- 75 Inlet
- 76 Inlet
- 77 Inlet
- 78 Inlet
- 79 Inlet
- 80 Inlet
- 81 Inlet
- 82 Inlet
- 83 Inlet
- 84 Inlet
- 85 Inlet
- 86 Inlet
- 87 Inlet
- 88 Inlet
- 89 Inlet
- 90 Inlet
- 91 Inlet
- 92 Inlet
- 93 Inlet
- 94 Inlet
- 95 Inlet
- 96 Inlet
- 97 Inlet
- 98 Inlet
- 99 Inlet
- 100 Inlet
- 101 Inlet
- 102 Inlet
- 103 Inlet
- 104 Inlet
- 105 Inlet
- 106 Inlet
- 107 Inlet
- 108 Inlet
- 109 Inlet
- 110 Inlet
- 111 Inlet
- 112 Inlet
- 113 Inlet
- 114 Inlet
- 115 Inlet
- 116 Inlet
- 117 Inlet
- 118 Inlet
- 119 Inlet
- 120 Inlet
- 121 Inlet
- 122 Inlet
- 123 Inlet
- 124 Inlet
- 125 Inlet
- 126 Inlet
- 127 Inlet
- 128 Inlet
- 129 Inlet
- 130 Inlet
- 131 Inlet
- 132 Inlet
- 133 Inlet
- 134 Inlet
- 135 Inlet
- 136 Inlet
- 137 Inlet
- 138 Inlet
- 139 Inlet
- 140 Inlet
- 141 Inlet
- 142 Inlet
- 143 Inlet
- 144 Inlet
- 145 Inlet
- 146 Inlet
- 147 Inlet
- 148 Inlet
- 149 Inlet
- 150 Inlet
- 151 Inlet
- 152 Inlet
- 153 Inlet
- 154 Inlet
- 155 Inlet
- 156 Inlet
- 157 Inlet
- 158 Inlet
- 159 Inlet
- 160 Inlet
- 161 Inlet
- 162 Inlet
- 163 Inlet
- 164 Inlet
- 165 Inlet
- 166 Inlet
- 167 Inlet
- 168 Inlet
- 169 Inlet
- 170 Inlet
- 171 Inlet
- 172 Inlet
- 173 Inlet
- 174 Inlet
- 175 Inlet
- 176 Inlet
- 177 Inlet
- 178 Inlet
- 179 Inlet
- 180 Inlet
- 181 Inlet
- 182 Inlet
- 183 Inlet
- 184 Inlet
- 185 Inlet
- 186 Inlet
- 187 Inlet
- 188 Inlet
- 189 Inlet
- 190 Inlet
- 191 Inlet
- 192 Inlet
- 193 Inlet
- 194 Inlet
- 195 Inlet
- 196 Inlet
- 197 Inlet
- 198 Inlet
- 199 Inlet
- 200 Inlet
- 201 Inlet
- 202 Inlet
- 203 Inlet
- 204 Inlet
- 205 Inlet
- 206 Inlet
- 207 Inlet
- 208 Inlet
- 209 Inlet
- 210 Inlet
- 211 Inlet
- 212 Inlet
- 213 Inlet
- 214 Inlet
- 215 Inlet
- 216 Inlet
- 217 Inlet
- 218 Inlet
- 219 Inlet
- 220 Inlet
- 221 Inlet
- 222 Inlet
- 223 Inlet
- 224 Inlet
- 225 Inlet
- 226 Inlet
- 227 Inlet
- 228 Inlet
- 229 Inlet
- 230 Inlet
- 231 Inlet
- 232 Inlet
- 233 Inlet
- 234 Inlet
- 235 Inlet
- 236 Inlet
- 237 Inlet
- 238 Inlet
- 239 Inlet
- 240 Inlet
- 241 Inlet
- 242 Inlet
- 243 Inlet
- 244 Inlet
- 245 Inlet
- 246 Inlet
- 247 Inlet
- 248 Inlet
- 249 Inlet
- 250 Inlet
- 251 Inlet
- 252 Inlet
- 253 Inlet
- 254 Inlet
- 255 Inlet
- 256 Inlet
- 257 Inlet
- 258 Inlet
- 259 Inlet
- 260 Inlet
- 261 Inlet
- 262 Inlet
- 263 Inlet
- 264 Inlet
- 265 Inlet
- 266 Inlet
- 267 Inlet
- 268 Inlet
- 269 Inlet
- 270 Inlet
- 271 Inlet
- 272 Inlet
- 273 Inlet
- 274 Inlet
- 275 Inlet
- 276 Inlet
- 277 Inlet
- 278 Inlet
- 279 Inlet
- 280 Inlet
- 281 Inlet
- 282 Inlet
- 283 Inlet

IAPMO RESEARCH AND TESTING, INC.

5001 E. Philadelphia Street, Ontario, CA 91761 • Phone (909) 472-4100 • Fax (909) 472-4244 • www.iapmo.org



CERTIFICATE OF LISTING

IAPMO Research and Testing, Inc. is a product certification body which tests and inspects samples taken from the supplier's stock or from the market or a combination of both to verify compliance to the requirements of applicable codes and standards. This activity is coupled with periodic surveillance of the supplier's factory and warehouses as well as the assessment of the supplier's Quality Assurance System. This listing is subject to the conditions set forth in the Characteristics below and is not to be construed as any recommendation, endorsement or guarantee by IAPMO Research and Testing, Inc. of the product acceptance by Authorities Having Jurisdiction.

Issued To:

QIANG YING HOSE FACTORY

BLOCK 1, NO. 225 JIAOXING NORTH ROAD, SHURUO TOWN, KAPING, GUANGDONG, CHINA

Product:

Drinking Water System Components - Health Effects

Products are in compliance with the following standard(s)
NSF/ANSI CAN 61-2018

File Number: N-12908
Effective Date: April 2021
Valid After: April 2026*



Susan O'Connell
Customer Product Certification Specialist

Chief Technical Service Officer

*This listing period is of indefinite or current listing. To re-verify listing status, visit the IAPMO R&T Product Listing Directory at pds.iapmo.org

This listing period is based on the date of the fourth evaluation of the product and may change in the future. In the event of material manufacturing changes, sampling or design without being approved or approval of the Product Certification Committee, or any violation of acceptance with applicable rules and standards or of inferior performance may be deemed sufficient cause for revocation of this listing. Production of an evaluation in this form for advertising purposes may be made only by specific permission of IAPMO Research and Testing, Inc. Any alteration of this certificate should be grounds for revocation of the listing. This document shall be reproduced in its entirety.

Page 1 of 4

IAPMO RESEARCH AND TESTING, INC.

CERTIFICATE OF LISTING

Issued To: QINANG YING HOSE FACTORY

Effective Date: April 2021

NSF/ANSI/CAN 6.1

File Number: N-12908

Product: Drinking Water System Components - Health Effects

Valid After: April 2026

This certificate is not evidence of current listing. To verify listing status, visit the IAPMO R&T Product Listing Directory at prod.usp.org

Models

Note: The following models are in compliance with NSF/ANSI/CAN 6.1, Section 9.

Flexible Braided Hose


| Legend Format | Description |
|--------------------------|--------------------------------|
| PEX-QY-BuB-C-*** | |
| B | Type of Nut/Connection Fitting |
| -F3/8 | |
| -F1/2 | |
| -F3/4 | |
| -F1S*1 | |
| -M3/8 | |
| -M1/2 | |
| -M3/4 | |
| -M1" | |
| -M1 1/2" | |
| -M1 1/4" | |
| -M1 3/4" | |
| -1/2NPSM | |
| -1NPSM | |
| -2NPSM | |
| -2NPS Quick Connect | |
| -gush fit | |
| -gush fit-three way | |
| C | Type of outer tube |
| -stainless steel braided | |
| -nylon braided | |
| *** | Length (in cm) |
| 20cm - 200cm | |

Page 1 of 4


[illegible]

BEFORE INSTALLATION

This product has been inspected and debugged by the factory to the best condition. Please do not disassemble and assemble it yourself.




Before installing the faucet, please be sure to remove sundries and sludge from the water pipe to prevent sundries from blocking the faucet.




1. Please read the manual firstly before installation;
2. Please check the condition of all the parts, and the installation tools are not included, please prepare it by yourself;
3. User manual includes matters needing attention during installation, please keep it properly;
4. The size chart in the manual is for reference only, please refer to the actual product that you receive.


Recommend Tools :




PTFE Tape



Hex Key




Slotted Screwdriver



Phillips Screwdriver

INSTALLATION DIMENSION

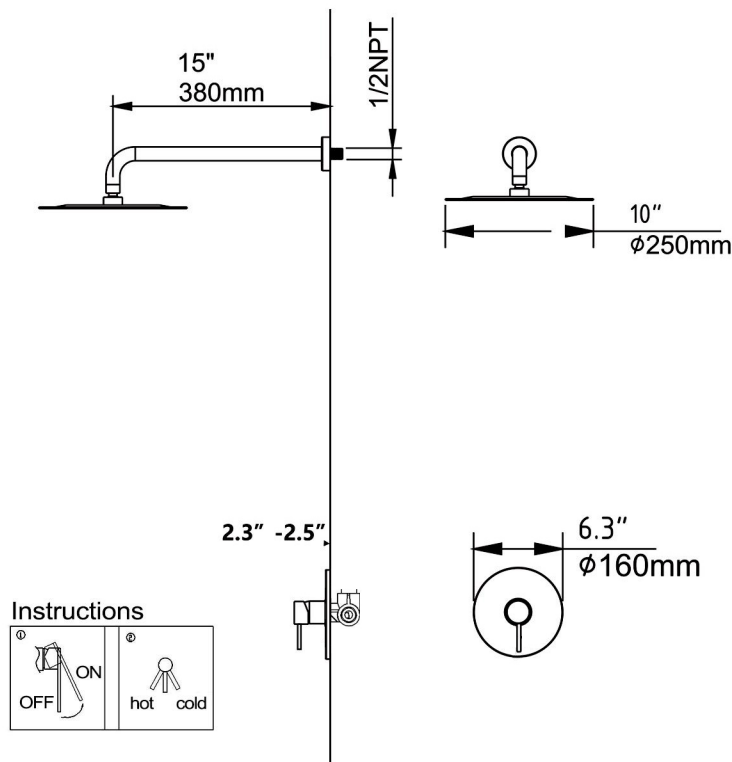



The picture is for reference only, you can install it according to your own requirements.

INSTALLATION STEPS


- 1.The sundries at the connection area must be cleared before installation to avoid blockage or leakage;
- 2.Connect the inlet pipe correctly as shown in the figure;
- 3.The maximum temperature of hot water is not higher than 80 °C (176°F);
- 4.Please contact seller for consultation if you need to install in other method.

①

Mark the location of screw holes on the wall, drill holes and install the water intake body

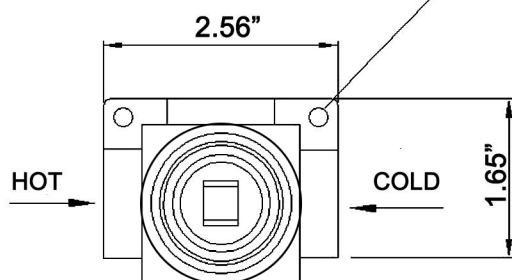


In the process of burying the wall, please do not remove the protective cover and avoid touching the copper sleeve.

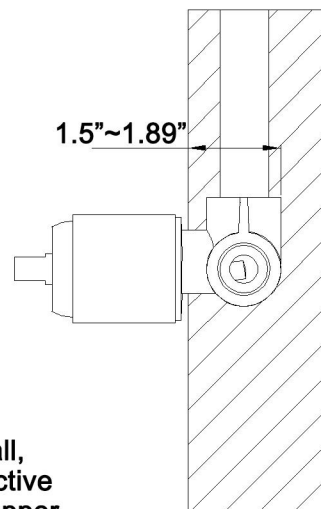

②Please install other parts in the order as shown in the figure below when the valve mounted to the wall:

- 1.Remove the lid of the Embedded Box;
- 2.Place the trim plate;
- 3.Mount the handles.

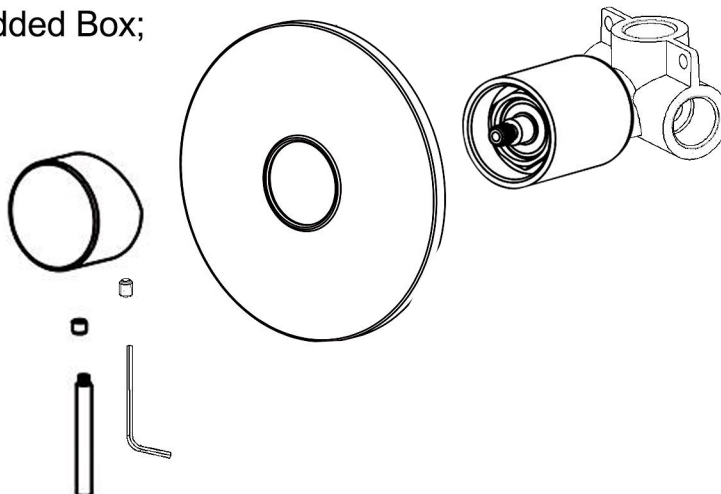

CLEANING CARE

In order to keep the appearance of faucet clean,bright and good performance, please take care of the faucet as follows;

- 1.Rinse with water only and dry with soff cotton cloth;
- 2.Use mild liquid and colorless glass cleaner to remove surface dirt and scale film, or use polish without abrasive effect;
- 3.Do not use abrasive deterfgent, polish, emery cloth, paper towel or scraper, etc.;
- 4.Do not use acid cleaner,or cleaner and soap with insoluble gran etc.;
- 5.In the process of use, mud my accumulate in the bubbler and make the water flow show, The bubbler can be unscrewed, rinsed with water, and then installed back in place.



